

PATIENT INFORMATION

Patient: _____
 Age: _____ Sex: _____ Height: _____ Weight: _____
 Diagnosis: _____

PRACTITIONER SHIPPING INFORMATION

Facility: _____
 Clinician: _____
 Address: _____
 City: _____
 State/Province/Region: _____ Zip: _____
 Country: _____
 Phone (Office): _____ Phone (Cell): _____
 Fax: _____ Email: _____

ORDER INFORMATION

PO#: _____


DEVICE SELECTION

Device Type:



Side: Left _____
 Right _____

Toe Out:



Toe Out Angle:

(+) Toe Out
 (-) Toe In

Left: _____
 Right: _____

Ankle Joint Alignment

Mechanical*

Tibial Torsion


Left: _____ °
 Right: _____ °

MEASUREMENTS

Anatomic Measurements

Inches

Centimeters

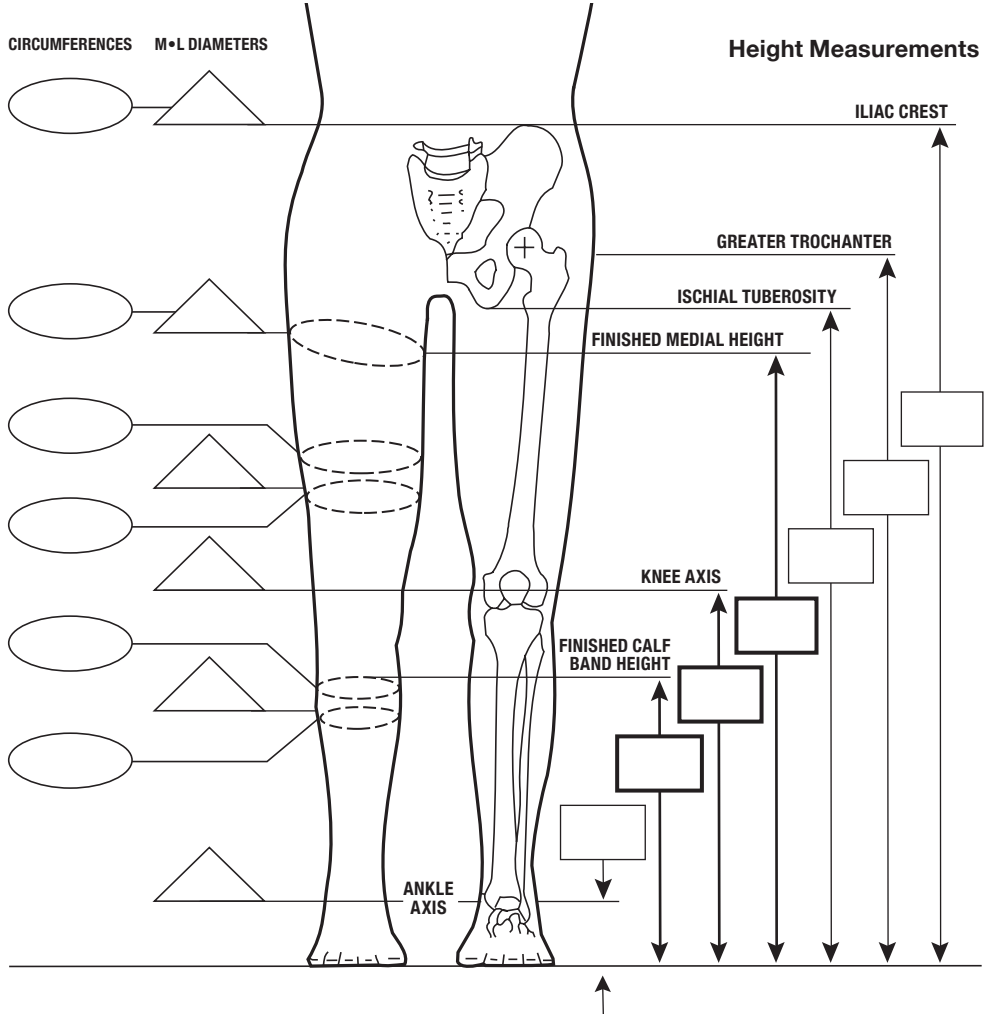

Note: If you don't choose an option, the * (default) option will be selected for you.

MATERIALS AND DESIGN

Footplate Options

- Shoe (provided by customer)
- UCBL (requires mold)

Ankle Control Strap Options

- Valgus Control T-Strap
- Varus Control T-Strap

Knee Control Strap Options

- 4-Buckle Strap
- 5-Buckle Strap

Leather Color Options

- Black***
- Beige
- Brown

Lacer Options

- Calf
 - Molded
 - Non-Molded
- Thigh
 - Molded
 - Non-Molded

COMPONENT SELECTION

Ankle Joints (select one)

- Standard Action (3025)
 - No Motion
 - Stop Motion _____° DF _____° PF
 - Free Motion
- Dorsiflexion Assist (3225)
- Double Action (SLM2825)

Ankle Joint Stirrup Options

- Solid Stirrup
 - Long
 - Wide
- Split Caliper

Knee Joints (select one)

- Alignment
 - Posterior Offset
- Lock Type
 - Free Motion
 - Ring Lock
 - Ball Catch
 - Lever Lock
 - Bail*
 - BLISS
 - HD Lever
 - Ratchet Lock
 - Bail*
 - BLISS
 - HD Lever
- Other (Specify) _____

Bar Material

- Aluminum
- Stainless Steel

Accessories

- Growth Extensions
- Quick Release
- Infra Patellar Strap
- Supra Patellar Strap
- Femoral Condyle Pad
 - Medial
 - Lateral

SPECIAL INSTRUCTIONS